

# ALCOTEST CHECKLIST

Municipality: EVESHAM TWP. Alcotest Ser. #: ARUL-0061

County: BURLINGTON Date of Calibration: 07-26-2010

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDUN S3-0311
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.  
Ser. #: DDUJ P2-110
- 4. **Digital Temperature Measuring System Report of Calibration.**  
Ser. #: 80614940
- 5.
  - A. Alcotest 7110 Calibration Record
  - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
  - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
  - D. **Alcotest Card** of operator/coordinator who performed tests.
  - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDWA P2-001
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
  - A. 0.04% Solution. 10 A 073
  - B. 0.08% Solution. 10 A 074
  - C. 0.10% Solution. 09 D 065
  - D. 0.16% Solution. 10 A 075
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
  - A. 0.04% used in Calibration/Linearity Testing. DDMK S3-0003
  - B. 0.08% used in Calibration/Linearity Testing. DDRK S3-0005
  - C. 0.10% used in Calibration/Linearity Testing DDUN S3-0311 [Same as instrument's CU34 unit].
  - D. 0.16% used in Calibration/Linearity Testing. DDRF S3-0009
- 8.
  - A. New Standard Solution Report following Calibration.
  - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
  - C. Certificate of Analysis 0.10% solution for same.  
Lot #: 09 B 063
  - D. Alcotest card of operator/coordinator who completed change.

Dräger safety

Alcotest<sup>®</sup> 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.


Certification Date:

SERIAL NUMBER:

7-21-2010

ARUL-0061

Dräger Safety Diagnostics, Inc.

  
\_\_\_\_\_



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDUN53-0311

Certification Date

Technician

Re-Certification Due Date

5/20/10

DM

5/20/11

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUJP2-110

5/19/10

5/19/11

Probe Value

104

Draeger Safety Diagnostics, Inc.  
Technical Service Department

DM



Calibration  
Certificate No. 1750.01

Calibration complies with ISO 9001  
ISO/IEC 17025 AND ANSI/NC SL Z540-1



Cert. No.: 4000-2023728

Traceable® Certificate of Calibration for Digital Thermometer

Instrument Identification:

Model: 61220-601      S/N: 80614940      Manufacturer : Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC191 Digital Thermometer	A79341 72310620/72310747	7/01/09	4000-1923693
Temperature Calibration Bath TC179 Digital Thermometer	A45240 22136727	5/16/09	4000-1882244
Temperature Probe	149	3/06/09	A82225037-3
Thermistor Module	A17118	11/15/08	A7831032
Temperature Calibration Bath TC218	A73332		

Certificate Information:

Technician: 68      Procedure: CAL-06      Cal Date: 11/04/08      Cal Due: 11/04/10  
Test Conditions: 23.5°C      44.0 %RH      1019 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±uc	TUR
°C		N.A.		0.001	0.000	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		25.004	24.999	Y	24.954	25.054	0.013	3.8:1
°C		N.A.		60.001	60.000	Y	59.951	60.051	0.018	2.8:1
°C		N.A.		100.001	99.999	Y	99.951	100.051	0.013	3.8:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Measurement Uncertainty; TUR=Test Uncertainty Ratio;  
Accuracy=±(Max-Min)/2; Date=MM/DD/YY

*Wallace Berry*  
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

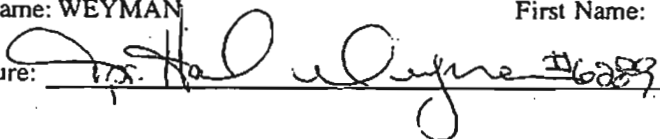
Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-AQ-HOU.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

# Alcotest 7110 Calibration Record


**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUL-0061  
Location: EVESHAM TOWNSHIP P.D.  
Calibration File No.: 00738 Calib. Date: 07/26/2010 Calib. No.: 00011  
Certification File No.: 00666 Cert. Date: 02/09/2010 Cert. No.: 00007  
Linearity File No.: 00667 Lin. Date: 02/09/2010 Lin. No.: 00007  
Solution File No.: 00737 Soln. Date: 07/21/2010 Soln. No.: 00079  
Sequential File No.: 00738 File Date: 07/26/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0311  
Control Solution %: 0.100% Expires: 04/22/2011  
Solution Control Lot: 09D065 Bottle No.: 0994

## Coordinator

Last Name: WEYMAN First Name: HAROLD MI: - -  
Signature:  #6289 Badge No.: 6289  
Date: 07/26/2010

\*Black Key Temperature Probe Serial.....# DDWAP2-001 H.W.  
\*Digital NIST Temperature Measuring System Serial.....# 8084940 H.W.



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Inspector, with full official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis which are analyzed in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUL-0061  
**Location:** EVESHAM TOWNSHIP P.D.  
**Calibration File No.:** 00738 **Calib. Date:** 07/26/2010 **Calib. No.:** 00011  
**Certification File No.:** 00739 **Cert. Date:** 07/26/2010 **Cert. No.:** 00008  
**Linearity File No.:** 00667 **Lin. Date:** 02/09/2010 **Lin. No.:** 00007  
**Solution File No.:** 00737 **Soln. Date:** 07/21/2010 **Soln. No.:** 00079  
**Sequential File No.:** 00739 **File Date:** 07/26/2010

**Calibrating Unit:** WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0311  
**Control Solution %:** 0.100% **Expires:** 04/22/2011  
**Solution Control Lot:** 09D065 **Bottle No.:** 0994

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:39D		
Control 1 EC	0.100%	13:39D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:40D		
Control 2 EC	0.100%	13:40D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41D		
Control 3 EC	0.100%	13:41D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:42D		

All tests within acceptable tolerance.

### Coordinator

Last Name: WEYMAN

First Name: HAROLD

Badge No.: 6289

Date: 07/26/2010

Signature: 

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUL-0061  
Location: EVESHAM TOWNSHIP P.D.  
Calibration File No.: 00738 Calib. Date: 07/26/2010 Calib. No.: 00011  
Certification File No.: 00739 Cert. Date: 07/26/2010 Cert. No.: 00008  
Linearity File No.: 00740 Lin. Date: 07/26/2010 Lin. No.: 00008  
Solution File No.: 00737 Soln. Date: 07/21/2010 Soln. No.: 00079  
Sequential File No.: 00740 File Date: 07/26/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0003  
Control Solution %: 0.040% Expires: 01/12/2012  
Solution Control Lot: 10A073 Bottle No.: 0303

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0005  
Control Solution %: 0.080% Expires: 01/15/2012  
Solution Control Lot: 10A074 Bottle No.: 0567

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRF S3-0009  
Control Solution %: 0.160% Expires: 01/21/2012  
Solution Control Lot: 10A075 Bottle No.: 0541

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:57D		
Control 1 EC	0.040%	13:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	13:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:59D		
Control 2 EC	0.040%	13:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	13:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:01D		
Control 3 EC	0.080%	14:01D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	14:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:03D		
Control 4 EC	0.080%	14:03D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	14:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 5 EC	0.162%	14:05D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.161%	14:05D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07D		
Control 6 EC	0.162%	14:07D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.162%	14:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:09D		

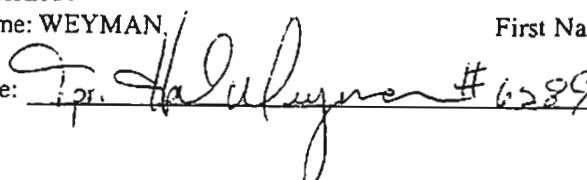
All tests within acceptable tolerance.

### Coordinator

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature:  #6289

Badge No.: 6289

Date: 07/26/2010

DEPARTMENT OF  
**Law and Public Safety**  
This is to certify that

**Harold Weyman**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL ANALYSES PURSUANT TO CHAPTER 140 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCO TEST 7110 MKII-C A METHOD TO DETERMINE INTOXICATION GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, ON 30th DAY OF MAY

TWO THOUSAND AND EIGHT


*[Signature]*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____	_____
2.	_____	_____	_____
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____





# CERTIFICATE

This is to certify that

**Harold Weyman**  
**Detective, #6289**

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and  
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: September 18, 2008

Instructor: Hansueli Ryser

**Dräger**

DEPARTMENT OF  
*Law and Public Safety*

This is to certify that

**Harold Weyman**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CLEARANCE TRAINING COURSES PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1964 IN THE OPERATION OF THE Breath Test Coordinator/Instructor  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, 5th DAY OF November

TWO THOUSAND AND Eight

*[Signature]*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____	_____
2.	_____	_____	_____
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____

ORIGINAL COURSE DATES \_\_\_\_\_

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____	_____
2.	_____	_____	_____
3.	_____	_____	_____
4.	_____	_____	_____
5.	_____	_____	_____
6.	_____	_____	_____
7.	_____	_____	_____
8.	_____	_____	_____
9.	_____	_____	_____

S.P. 2938 (Rev. 06/03)

DEPARTMENT OF  
*Law and Public Safety*  
This is to certify that

HAROLD WEYMAN

NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT BREATHALYZER ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE BREATHALYZER A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 13th DAY OF August

TWO THOUSAND AND Four  
  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

**Dräger**safety

**ALCOTEST® 7110 TEMPERATURE PROBE**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAPJ-001

Certification date:

2-3-10

Next Certification due:

2-3-11

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

MM



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

PAULA T. DOW  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

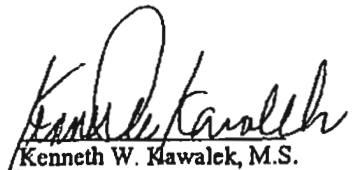
MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/2/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A073


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0481 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 12, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Krawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of February, 2010.

  
 Notary

Linda L. Desantis  
 Notary Public, New Jersey  
 Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/3/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A074

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0954 to 0.0958 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 15, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kalvarek, M.S.
Kenneth W. Kalvarek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.

Handwritten signature of Linda L. Decaris
Notary

Linda L. Decaris
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 5/08/2009

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09D065

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1201 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 22, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of May, 2009.

Notary

Linda L. DeSantis  
 My Commission  
 Expires Aug. 17, 2009





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

PAULA T. DOW  
 Acting Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.


MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/4/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A075


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1913 to 0.1919 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 21, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Kawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of February, 2010.

  
 Notary

Linda L. Desantis  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable







**Drägersafety**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK II A

Other: \_\_\_\_\_

Serial Number:

DDMKS3-0003

Certification Date

Technician

Re-Certification Due Date

2/3/10

z.m

2/3/11



**Dräger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRK 53-0005

Certification Date

Technician

Re-Certification Due Date

2/3/10

am

2/3/11



**Drägersafety**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRF53 - 0009

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
<b>Location:</b>	EVESHAM TOWNSHIP P.D.	
<b>Calibration File No.:</b>	00738	<b>Calib. Date:</b> 07/26/2010
<b>Certification File No.:</b>	00739	<b>Calib. No.:</b> 00011
<b>Linearity File No.:</b>	00740	<b>Cert. Date:</b> 07/26/2010
<b>Solution File No.:</b>	00741	<b>Cert. No.:</b> 00008
<b>Sequential File No.:</b>	00741	<b>Lin. Date:</b> 07/26/2010
		<b>Lin. No.:</b> 00008
		<b>Soln. Date:</b> 07/26/2010
		<b>Soln. No.:</b> 00080
		<b>File Date:</b> 07/26/2010
<b>Calibrating Unit:</b>	WET	<b>Model No.:</b> CU-34
<b>Control Solution %:</b>	0.100%	<b>Serial No.:</b> DDUN S3-0311
<b>Solution Control Lot:</b>	09B063	<b>Expires:</b> 02/02/2011
		<b>Bottle No.:</b> 0953

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:17D		
Control 1 EC	0.101%	15:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18D		
Control 2 EC	0.101%	15:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:19D		
Control 3 EC	0.101%	15:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDJJP2 - 1104110

Changed By:

Last Name: WEYMAN

First Name: HAROLD

MI: -

Signature:

*H. Weyman #6289*

Badge No.: 6289

Date: 07/26/2010



JON S. CORZINE  
Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
Post Office Box 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

ANNE MILGRAM  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/27/2009

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09B063

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1199 to 0.1205 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 2, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

*Ajit R. Tungare*

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 5 day of March, 2009.

*John R. Leaver*  
Notary

JOHN R. LEAVER  
NOTARY PUBLIC STATE OF NEW JERSEY  
MY COMMISSION EXPIRES 12/14/2012

