

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 07/24/2012
Certification File No.:	00010	Cert. No.: 00006
Linearity File No.:	00011	Cert. Date: 07/24/2012
Solution File No.:	00035	Lin. Date: 07/24/2012
Sequential File No.:	00035	Lin. No.: 00001
		Soln. Date: 10/21/2012
		Soln. No.: 00007
		File Date: 10/21/2012

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDDC-0001
Control Solution %:	0.100%			Expires:	09/15/2013
Solution Control Lot:	11I095			Bottle No.:	0798

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:41D		
Control 1 EC	0.100%	20:41D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	20:41D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:42D		
Control 2 EC	0.099%	20:43D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	20:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:43D		
Control 3 EC	0.100%	20:44D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:44D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: _____

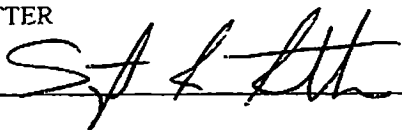

Badge No.: 63

Date: 10/21/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00006
Calibration File No.:	00009	Cert. Date:	07/24/2012
Certification File No.:	00010	Lin. Date:	07/24/2012
Linearity File No.:	00011	Soln. Date:	10/13/2012
Solution File No.:	00032	File Date:	10/13/2012
Sequential File No.:	00032		

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDDC-0001
Control Solution %:	0.100%			Expires:	09/15/2013
Solution Control Lot:	111095			Bottle No.:	0797

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:09D		
Control 1 EC	0.103%	09:10D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	09:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		
Control 2 EC	0.103%	09:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	09:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:12D		
Control 3 EC	0.103%	09:13D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	09:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature: 

Badge No.: 104

Date: 10/13/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00009	Calib. Date: 07/24/2012
Certification File No.:	00010	Calib. No.: 00006
Linearity File No.:	00011	Cert. Date: 07/24/2012
Solution File No.:	00025	Cert. No.: 00002
Sequential File No.:	00025	Lin. Date: 07/24/2012
		Lin. No.: 00001
		Soln. Date: 09/15/2012
		Soln. No.: 00005
		File Date: 09/15/2012

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDDC-0001
Control Solution %:	0.100%		Expires: 09/15/2013
Solution Control Lot:	111095		Bottle No.: 0792

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:24D		
Control 1 EC	0.097%	09:24D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:24D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		
Control 2 EC	0.098%	09:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26D		
Control 3 EC	0.099%	09:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature: _____

PR Andrew Dougherty 104

Badge No.: 104

Date: 09/15/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00009	Calib. Date:	07/24/2012
Certification File No.:	00010	Cert. Date:	07/24/2012
Linearity File No.:	00011	Lin. Date:	07/24/2012
Solution File No.:	00017	Soln. Date:	08/17/2012
Sequential File No.:	00017	File Date:	08/17/2012

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDDC-0001
Control Solution %:	0.100%			Expires:	09/15/2013
Solution Control Lot:	111095			Bottle No.:	0782

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:27D		
Control 1 EC	0.101%	00:28D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	00:28D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:28D		
Control 2 EC	0.101%	00:29D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	00:29D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:30D		
Control 3 EC	0.100%	00:30D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	00:30D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:31D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: DOLPHIN

First Name: SEAN

MI: P

Signature: _____

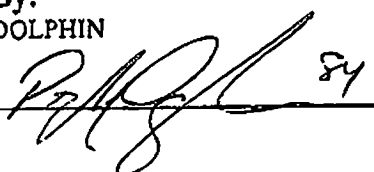

Badge No.: 84

Date: 08/17/2012