

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 01089 **Calib. Date:** 05/23/2012 **Calib. No.:** 00015
Certification File No.: 01090 **Cert. Date:** 05/23/2012 **Cert. No.:** 00012
Linearity File No.: 01091 **Lin. Date:** 05/23/2012 **Lin. No.:** 00012
Solution File No.: 01162 **Soln. Date:** 10/28/2012 **Soln. No.:** 00128
Sequential File No.: 01162 **File Date:** 10/28/2012

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0310
Control Solution %: 0.100% **Expires:** 09/15/2013
Solution Control Lot: 111095 **Bottle No.:** 0795

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:42S		
Control 1 EC	0.099%	10:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43S		
Control 2 EC	0.096%	10:44S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45S		
Control 3 EC	0.097%	10:45S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	10:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:46S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature: _____

PTC Andrew B Dougherty 104

Badge No.: 104

Date: 10/28/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	01089	Calib. Date:	05/23/2012
Certification File No.:	01090	Cert. Date:	05/23/2012
Linearity File No.:	01091	Lin. Date:	05/23/2012
Solution File No.:	01157	Soln. Date:	10/22/2012
Sequential File No.:	01157	File Date:	10/22/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0799

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:52D		
Control 1 EC	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 2 EC	0.097%	09:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	09:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		
Control 3 EC	0.097%	09:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	09:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: _____

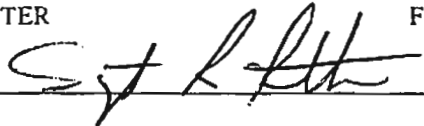

Badge No.: 63

Date: 10/22/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00015
Calibration File No.:	01089	Cert. Date:	05/23/2012
Certification File No.:	01090	Lin. Date:	05/23/2012
Linearity File No.:	01091	Soln. Date:	10/13/2012
Solution File No.:	01153	File Date:	10/13/2012
Sequential File No.:	01153		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0793

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:17D		
Control 1 EC	0.097%	09:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	09:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18D		
Control 2 EC	0.097%	09:19D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		
Control 3 EC	0.097%	09:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOUGERTY

First Name: ANDREW

MI: B

Signature:

Badge No.: 104

Date: 10/13/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	01089	Calib. Date:	05/23/2012
Certification File No.:	01090	Cert. No.:	00015
Linearity File No.:	01091	Cert. Date:	05/23/2012
Solution File No.:	01145	Lin. No.:	00012
Sequential File No.:	01145	Soln. Date:	09/15/2012
		Soln. No.:	00123
		File Date:	09/15/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0786

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:19D		
Control 1 EC	0.098%	09:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:20D		
Control 2 EC	0.098%	09:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:21D		
Control 3 EC	0.097%	09:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOUGHERTY

First Name: ANDREW

MI: B

Signature: 

Badge No.: 104

Date: 09/15/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 01089 **Calib. Date:** 05/23/2012 **Calib. No.:** 00015
Certification File No.: 01090 **Cert. Date:** 05/23/2012 **Cert. No.:** 00012
Linearity File No.: 01091 **Lin. Date:** 05/23/2012 **Lin. No.:** 00012
Solution File No.: 01135 **Soln. Date:** 08/16/2012 **Soln. No.:** 00122
Sequential File No.: 01135 **File Date:** 08/16/2012

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDUN S3-0310
Control Solution %: 0.100% **Expires:** 09/15/2013
Solution Control Lot: 111095 **Bottle No.:** 0787

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:47D		
Control 1 EC	0.096%	23:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	23:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:48D		
Control 2 EC	0.097%	23:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	23:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50D		
Control 3 EC	0.097%	23:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	23:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DOLPHIN

First Name: SEAN

MI: P

Signature: 

Badge No.: 84

Date: 08/16/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	01089	Calib. Date: 05/23/2012
Certification File No.:	01090	Calib. No.: 00015
Linearity File No.:	01091	Cert. Date: 05/23/2012
Solution File No.:	01126	Cert. No.: 00012
Sequential File No.:	01126	Lin. Date: 05/23/2012
		Lin. No.: 00012
		Soln. Date: 07/20/2012
		Soln. No.: 00121
		File Date: 07/20/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	111095	Expires: 09/15/2013
		Bottle No.: 0788

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:28D		
Control 1 EC	0.098%	08:28D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:28D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:29D		
Control 2 EC	0.098%	08:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:30D		
Control 3 EC	0.099%	08:31D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:31D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: 

Badge No.: 2296

Date: 07/20/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	01089	Calib. Date:	05/23/2012
Certification File No.:	01090	Cert. Date:	05/23/2012
Linearity File No.:	01091	Lin. Date:	05/23/2012
Solution File No.:	01102	Soln. Date:	06/08/2012
Sequential File No.:	01102	File Date:	06/08/2012

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUN S3-0310
Control Solution %:	0.100%			Expires:	09/15/2013
Solution Control Lot:	111095			Bottle No.:	0779

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:04D		
Control 1 EC	0.098%	13:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	13:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:05D		
Control 2 EC	0.097%	13:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:06D		
Control 3 EC	0.097%	13:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	13:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: PTL [Handwritten Signature]

Badge No.: 2296

Date: 06/08/2012

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 01089 Calib. Date: 05/23/2012 Calib. No.: 00015
Certification File No.: 01090 Cert. Date: 05/23/2012 Cert. No.: 00012
Linearity File No.: 01091 Lin. Date: 05/23/2012 Lin. No.: 00012
Solution File No.: 01101 Soln. Date: 06/08/2012 Soln. No.: 00118
Sequential File No.: 01101 File Date: 06/08/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 09/15/2013
Solution Control Lot: 111095 Bottle No.: 0778

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:39D		
Control 1 EC	0.088%	11:40D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.088%	11:40D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:41D		
Control 2 EC	0.088%	11:42D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.089%	11:42D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:43D		
Control 3 EC	0.091%	11:43D	34.0°C	CONTROL TEST FAILED
Control 3 IR	0.093%	11:43D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	11:45D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: PTL [Signature] 96

Badge No.: 2296

Date: 06/08/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	01089	Calib. Date:	05/23/2012
Certification File No.:	01090	Cert. Date:	05/23/2012
Linearity File No.:	01091	Lin. Date:	05/23/2012
Solution File No.:	01100	Soln. Date:	06/08/2012
Sequential File No.:	01100	File Date:	06/08/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0778

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:03D		
Control 1 EC	-.---%	10:03D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	10:03D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: PTL [Handwritten Signature] # 96

Badge No.: 2296

Date: 06/08/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	01016	Calib. No.: 00014
Certification File No.:	01017	Cert. No.: 00011
Linearity File No.:	01018	Lin. No.: 00011
Solution File No.:	01085	Soln. No.: 00115
Sequential File No.:	01085	File Date: 05/12/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	111095	Expires: 09/15/2013
		Bottle No.: 1400

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:53D		
Control 1 EC	0.099%	11:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		
Control 2 EC	0.098%	11:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56D		
Control 3 EC	0.098%	11:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: NIJI

First Name: DAVID

MI: R

Signature: _____

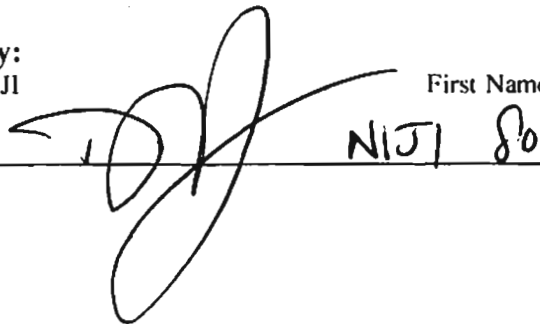

Badge No.: 80

Date: 05/12/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00014
Calibration File No.:	01016	Cert. Date:	11/28/2011
Certification File No.:	01017	Lin. Date:	11/28/2011
Linearity File No.:	01018	Soln. Date:	04/20/2012
Solution File No.:	01075	File Date:	04/20/2012
Sequential File No.:	01075		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0783

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:08D		
Control 1 EC	0.099%	15:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:09D		
Control 2 EC	0.099%	15:10D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	15:10D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:10D		
Control 3 EC	0.099%	15:11D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:12D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 04/20/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	01016	Calib. Date: 11/28/2011
Certification File No.:	01017	Calib. No.: 00014
Linearity File No.:	01018	Cert. Date: 11/28/2011
Solution File No.:	01069	Cert. No.: 00011
Sequential File No.:	01069	Lin. Date: 11/28/2011
		Lin. No.: 00011
		Soln. Date: 03/22/2012
		Soln. No.: 00113
		File Date: 03/22/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0310
Solution Control Lot:	111095	Expires: 09/15/2013
		Bottle No.: 0780

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:03S		
Control 1 EC	0.099%	12:04S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		
Control 2 EC	0.099%	12:05S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06S		
Control 3 EC	0.099%	12:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

M1: F

Signature: PTL  # 96

Badge No.: 2296

Date: 03/22/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00014
Calibration File No.:	01016	Cert. Date:	11/28/2011
Certification File No.:	01017	Lin. Date:	11/28/2011
Linearity File No.:	01018	Soln. Date:	02/28/2012
Solution File No.:	01056	File Date:	02/28/2012
Sequential File No.:	01056		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0785

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:02S		
Control 1 EC	0.100%	10:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:03S		
Control 2 EC	0.100%	10:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:04S		
Control 3 EC	0.099%	10:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: _____

PTL [Signature] # 96

Badge No.: 2296

Date: 02/28/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUL-0061
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00014
Calibration File No.:	01016	Calib. Date:	11/28/2011
Certification File No.:	01017	Cert. Date:	11/28/2011
Linearity File No.:	01018	Lin. Date:	11/28/2011
Solution File No.:	01045	Soln. Date:	01/28/2012
Sequential File No.:	01045	File Date:	01/28/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0310
Solution Control Lot:	111095	Expires:	09/15/2013
		Bottle No.:	0790

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:29S		
Control 1 EC	0.099%	09:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31S		
Control 2 EC	0.097%	09:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:32S		
Control 3 EC	0.098%	09:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ARMSTRONG

First Name: JACK

MI: J

Signature: _____

Badge No.: 93

Date: 01/28/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUL-0061
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 01016 Calib. Date: 11/28/2011 Calib. No.: 00014
Certification File No.: 01017 Cert. Date: 11/28/2011 Cert. No.: 00011
Linearity File No.: 01018 Lin. Date: 11/28/2011 Lin. No.: 00011
Solution File No.: 01032 Soln. Date: 01/04/2012 Soln. No.: 00110
Sequential File No.: 01032 File Date: 01/04/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0310
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 1016

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:12S		
Control 1 EC	0.100%	09:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13S		
Control 2 EC	0.099%	09:14S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:14S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14S		
Control 3 EC	0.098%	09:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LACARTE

First Name: BRUCE

MI: F

Signature: _____



Badge No.: 31

Date: 01/04/2012