

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00246	Calib. Date: 08/20/2014
Certification File No.:	00247	Calib. No.: 00011
Linearity File No.:	00248	Cert. Date: 08/20/2014
Solution File No.:	00271	Cert. No.: 00007
Sequential File No.:	00271	Lin. Date: 08/20/2014
		Lin. No.: 00006
		Soln. Date: 11/18/2014
		Soln. No.: 00050
		File Date: 11/18/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0122
Solution Control Lot:	13C111	Expires: 03/12/2015
		Bottle No.: 0996

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:52S		
Control 1 EC	0.104%	08:53S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	08:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53S		
Control 2 EC	0.103%	08:54S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.104%	08:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:55S		
Control 3 EC	0.103%	08:55S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	08:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:56S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: -

Signature: _____

Officer Thomas Magee

Badge No.: 50

Date: 11/18/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00246	Calib. Date: 08/20/2014
Certification File No.:	00247	Cert. No.: 00011
Linearity File No.:	00248	Cert. Date: 08/20/2014
Solution File No.:	00270	Lin. No.: 00007
Sequential File No.:	00270	Lin. Date: 08/20/2014
		Lin. No.: 00006
		Soln. Date: 11/17/2014
		Soln. No.: 00049
		File Date: 11/17/2014

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0122
Control Solution %:	0.100%			Expires:	03/12/2015
Solution Control Lot:	13C111			Bottle No.:	0995

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:44S		
Control 1 EC	-.---%	07:44S	19.7°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	07:44S	19.7°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: -

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 11/17/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00246	Calib. Date: 08/20/2014
Certification File No.:	00247	Calib. No.: 00011
Linearity File No.:	00248	Cert. Date: 08/20/2014
Solution File No.:	00257	Cert. No.: 00007
Sequential File No.:	00257	Lin. Date: 08/20/2014
		Lin. No.: 00006
		Soln. Date: 10/18/2014
		Soln. No.: 00048
		File Date: 10/18/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0122
Solution Control Lot:	13C111	Expires: 03/12/2015
		Bottle No.: 0007

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:43D		
Control 1 EC	0.101%	02:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	02:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:44D		
Control 2 EC	0.101%	02:45D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	02:45D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:45D		
Control 3 EC	0.101%	02:46D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	02:46D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: -

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 10/18/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00011
Calibration File No.:	00246	Calib. Date:	08/20/2014
Certification File No.:	00247	Cert. Date:	08/20/2014
Linearity File No.:	00248	Lin. Date:	08/20/2014
Solution File No.:	00253	Soln. Date:	09/18/2014
Sequential File No.:	00253	File Date:	09/18/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0122
Solution Control Lot:	13C111	Expires:	03/12/2015
		Bottle No.:	0004

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:04D		
Control 1 EC	0.100%	14:04D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 2 EC	0.099%	14:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:06D		
Control 3 EC	0.100%	14:07D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	14:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Temperature Probe Serial Number: DDEEP2 - 032 MA

Changed By:

Last Name: GONCALVES

First Name: MICHELLE

MI: L

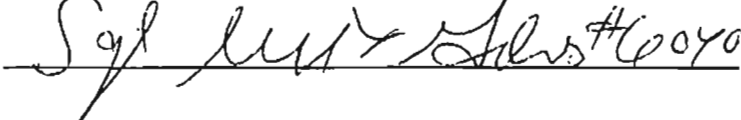Signature: 

Badge No.: 6040

Date: 09/18/2014



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDUKS3-022

Certification Date

9-12-14

Technician

BC

Re-Certification Due Date

9-12-15



Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDEE P2-032

Certification date:

9-12-14

Next Certification due:

9-12-15

Probe Value

104

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00010
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. Date:	02/25/2014
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00245	Soln. Date:	08/17/2014
Sequential File No.:	00245	File Date:	08/17/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1299

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:09D		
Control 1 EC	0.096%	20:10D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	20:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:10D		
Control 2 EC	0.096%	20:11D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	20:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:12D		
Control 3 EC	0.096%	20:12D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	20:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:13D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: PTL. [Handwritten Signature] #96

Badge No.: 2296

Date: 08/17/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. No.:	00010
Linearity File No.:	00185	Cert. Date:	02/25/2014
Solution File No.:	00238	Lin. No.:	00005
Sequential File No.:	00238	Lin. Date:	02/25/2014
		Soln. Date:	07/27/2014
		Soln. No.:	00044
		File Date:	07/27/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1298

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	21:52D		
Control 1 EC	0.096%	21:53D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	21:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:53D		
Control 2 EC	0.096%	21:54D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	21:54D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:55D		
Control 3 EC	0.096%	21:55D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.096%	21:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	21:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FITZPATRICK

First Name: BRIAN

M1: D

Signature: _____

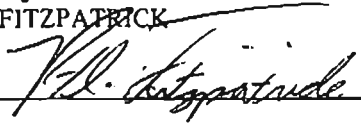

Badge No.: 2286

Date: 07/27/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00010
Calibration File No.:	00183	Cert. Date:	02/25/2014
Certification File No.:	00184	Lin. Date:	02/25/2014
Linearity File No.:	00185	Soln. Date:	07/20/2014
Solution File No.:	00235	File Date:	07/20/2014
Sequential File No.:	00235		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1297

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	17:00D		
Control 1 EC	0.097%	17:01D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	17:01D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01D		
Control 2 EC	0.096%	17:02D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	17:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:03D		
Control 3 EC	0.096%	17:03D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	17:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SCAMBIA

First Name: MARC

MI: F

Signature: PTL. 2  #96

Badge No.: 2296

Date: 07/20/2014

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARDC-0066
Location: EVESHAM TOWNSHIP P.D.
Calibration File No.: 00183 Calib. Date: 02/25/2014 Calib. No.: 00010
Certification File No.: 00184 Cert. Date: 02/25/2014 Cert. No.: 00006
Linearity File No.: 00185 Lin. Date: 02/25/2014 Lin. No.: 00005
Solution File No.: 00230 Soln. Date: 06/20/2014 Soln. No.: 00042
Sequential File No.: 00230 File Date: 06/20/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDDC-0001
Control Solution %: 0.100% Expires: 07/18/2015
Solution Control Lot: 13G115 Bottle No.: 1286

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:11D		
Control 1 EC	0.096%	11:11D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	11:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12D		
Control 2 EC	0.096%	11:13D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:13D		
Control 3 EC	0.096%	11:14D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	11:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:15D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

M1: A

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 06/20/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	Calib. No.:	00010
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. Date:	02/25/2014
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00225	Soln. Date:	06/16/2014
Sequential File No.:	00225	File Date:	06/16/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1295

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:05D		
Control 1 EC	0.097%	08:06D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	08:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:07D		
Control 2 EC	0.096%	08:07D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.096%	08:07D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 3 EC	0.096%	08:09D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	08:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: A

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 06/16/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. No.:	00006
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00220	Soln. No.:	00040
Sequential File No.:	00220	File Date:	05/30/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1289

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:15D		
Control 1 EC	0.097%	20:16D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.097%	20:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:16D		
Control 2 EC	0.096%	20:17D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	20:17D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:18D		
Control 3 EC	0.096%	20:18D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	20:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: A

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 05/30/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00183	Calib. Date: 02/25/2014
Certification File No.:	00184	Calib. No.: 00010
Linearity File No.:	00185	Cert. Date: 02/25/2014
Solution File No.:	00215	Cert. No.: 00006
Sequential File No.:	00215	Lin. Date: 02/25/2014
		Lin. No.: 00005
		Soln. Date: 05/07/2014
		Soln. No.: 00039
		File Date: 05/07/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDDC-0001
Solution Control Lot:	13G115	Expires: 07/18/2015
		Bottle No.: 1292

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50D		
Control 1 EC	0.098%	13:51D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:51D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51D		
Control 2 EC	0.097%	13:52D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:52D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53D		
Control 3 EC	0.097%	13:53D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:53D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAGEE

First Name: THOMAS

MI: A

Signature: Officer Thomas Magee #50

Badge No.: 50

Date: 05/07/2014

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MK111-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00183	Calib. Date: 02/25/2014 Calib. No.: 00010
Certification File No.:	00184	Cert. Date: 02/25/2014 Cert. No.: 00006
Linearity File No.:	00185	Lin. Date: 02/25/2014 Lin. No.: 00005
Solution File No.:	00207	Soln. Date: 04/20/2014 Soln. No.: 00038
Sequential File No.:	00207	File Date: 04/20/2014

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDDC-0001
Control Solution %:	0.100%		Expires: 07/18/2015
Solution Control Lot:	13G115		Bottle No.: 1290

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:07D		
Control 1 EC	0.096%	08:08D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	08:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 2 EC	0.096%	08:09D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:09D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		
Control 3 EC	0.097%	08:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MANCINI

First Name: MICHAEL

MI: S

Signature: _____

Michael Mancini #94

Badge No.: 94

Date: 04/20/2014

Calibrating Unit


New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. Date:	02/25/2014
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00199	Soln. Date:	04/05/2014
Sequential File No.:	00199	File Date:	04/05/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1285

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:30S		
Control 1 EC	0.097%	02:31S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	02:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:31S		
Control 2 EC	0.096%	02:32S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:32S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:33S		
Control 3 EC	0.096%	02:34S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:34S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:34S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

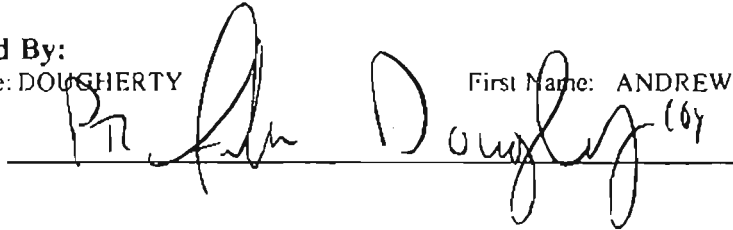Changed By:
 Last Name: DOUGHERTY First Name: ANDREW MI: B
 Signature:  Badge No.: 104
 Date: 04/05/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. Date:	02/25/2014
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00194	Soln. Date:	03/28/2014
Sequential File No.:	00194	File Date:	03/28/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1284

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:19S		
Control 1 EC	0.098%	13:20S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:20S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:21S		
Control 2 EC	0.097%	13:21S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22S		
Control 3 EC	0.097%	13:23S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:23S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:23S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: _____

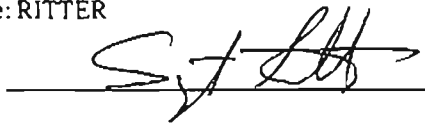

Badge No.: 63

Date: 03/28/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.		
Calibration File No.:	00183	Calib. Date:	02/25/2014
Certification File No.:	00184	Cert. Date:	02/25/2014
Linearity File No.:	00185	Lin. Date:	02/25/2014
Solution File No.:	00186	Soln. Date:	02/25/2014
Sequential File No.:	00186	File Date:	02/25/2014
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDDC-0001
Solution Control Lot:	13G115	Expires:	07/18/2015
		Bottle No.:	1279

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:29S		
Control 1 EC	0.100%	16:30S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	16:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:31S		
Control 2 EC	0.099%	16:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:32S		
Control 3 EC	0.099%	16:33S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:34S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDLJPI - 0033 ML

Changed By:

Last Name: GONCALVES First Name: MICHELLE MI: L

Signature: A/Sgt Helms #6040 Badge No.: 6040 Date: 02/25/2014



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 7/29/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13G115

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1213 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 18, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alabiue, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 7th day of August, 2013.

Linda L. DeSantis
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKJJ1-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00152	Calib. Date: 10/07/2013
Certification File No.:	00153	Calib. No.: 00009
Linearity File No.:	00154	Cert. Date: 10/07/2013
Solution File No.:	00182	Cert. No.: 00005
Sequential File No.:	00182	Lin. Date: 10/07/2013
		Lin. No.: 00004
		Soln. Date: 02/20/2014
		Soln. No.: 00033
		File Date: 02/20/2014

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDDC-0001
Control Solution %:	0.100%		Expires: 07/18/2015
Solution Control Lot:	13G115		Bottle No.: 1278

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:13S		
Control 1 EC	0.103%	11:13S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:13S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:14S		
Control 2 EC	0.100%	11:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	11:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:16S		
Control 3 EC	0.101%	11:16S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:17S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: _____

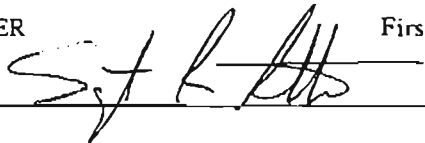

Badge No.: 63

Date: 02/20/2014

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARDC-0066
Location:	EVESHAM TOWNSHIP P.D.	
Calibration File No.:	00152	Calib. Date: 10/07/2013
Certification File No.:	00153	Calib. No.: 00009
Linearity File No.:	00154	Cert. Date: 10/07/2013
Solution File No.:	00179	Cert. No.: 00005
Sequential File No.:	00179	Lin. Date: 10/07/2013
		Lin. No.: 00004
		Soln. Date: 01/21/2014
		Soln. No.: 00032
		File Date: 01/21/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDDC-0001
Solution Control Lot:	13G115	Expires: 07/18/2015
		Bottle No.: 1277

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:05S		
Control 1 EC	0.102%	10:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	10:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06S		
Control 2 EC	0.101%	10:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		
Control 3 EC	0.101%	10:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: RITTER

First Name: RONALD

MI: C

Signature: _____



Badge No.: 63

Date: 01/21/2014