

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01729	Calib. Date: 12/03/2013
Certification File No.:	01730	Calib. No.: 00028
Linearity File No.:	01731	Cert. Date: 12/03/2013
Solution File No.:	01740	Cert. No.: 00019
Sequential File No.:	01740	Lin. Date: 12/03/2013
		Lin. No.: 00018
		Soln. Date: 12/13/2013
		Soln. No.: 00189
		File Date: 12/13/2013

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUL S3-0163
Control Solution %: 0.100%		Expires: 12/26/2014
Solution Control Lot: 12L109		Bottle No.: 0420

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:59S		
Control 1 EC	0.099%	12:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01S		
Control 2 EC	0.098%	12:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02S		
Control 3 EC	0.098%	12:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	12:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

 63200

Badge No.: 3200

Date: 12/13/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01619	Calib. Date: 06/19/2013
Certification File No.:	01620	Calib. No.: 00027
Linearity File No.:	01621	Cert. Date: 06/19/2013
Solution File No.:	01714	Cert. No.: 00018
Sequential File No.:	01714	Lin. Date: 06/19/2013
		Lin. No.: 00017
		Soln. Date: 11/14/2013
		Soln. No.: 00187
		File Date: 11/14/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 04/25/2014
Solution Control Lot:	12D101		Bottle No.: 0571

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:00S		
Control 1 EC	0.101%	15:00S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:01S		
Control 2 EC	0.100%	15:02S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:03S		
Control 3 EC	0.100%	15:03S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 11/14/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01619	Calib. Date: 06/19/2013
Certification File No.:	01620	Calib. No.: 00027
Linearity File No.:	01621	Cert. Date: 06/19/2013
Solution File No.:	01699	Cert. No.: 00018
Sequential File No.:	01699	Lin. Date: 06/19/2013
		Lin. No.: 00017
		Soln. Date: 10/24/2013
		Soln. No.: 00186
		File Date: 10/24/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	12D101	Expires: 04/25/2014
		Bottle No.: 0572

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:16D		
Control 1 EC	0.099%	08:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18D		
Control 2 EC	0.098%	08:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:19D		
Control 3 EC	0.098%	08:20D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MCBRIDE

First Name: STEPHEN

MI: J

Signature: \_\_\_\_\_

Badge No.: 3202

Date: 10/24/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT	
Calibration File No.:	01619	Calib. Date: 06/19/2013
Certification File No.:	01620	Calib. No.: 00027
Linearity File No.:	01621	Cert. Date: 06/19/2013
Solution File No.:	01683	Cert. No.: 00018
Sequential File No.:	01683	Lin. Date: 06/19/2013
		Lin. No.: 00017
		Soln. Date: 10/04/2013
		Soln. No.: 00185
		File Date: 10/04/2013

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUK S3-0133
Solution Control Lot:	12D101	Expires: 04/25/2014
		Bottle No.: 0556

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:08D		
Control 1 EC	0.101%	10:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09D		
Control 2 EC	0.100%	10:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:10D		
Control 3 EC	0.100%	10:11D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	10:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 10/04/2013

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01619 Calib. Date: 06/19/2013 Calib. No.: 00027  
Certification File No.: 01620 Cert. Date: 06/19/2013 Cert. No.: 00018  
Linearity File No.: 01621 Lin. Date: 06/19/2013 Lin. No.: 00017  
Solution File No.: 01669 Soln. Date: 09/12/2013 Soln. No.: 00184  
Sequential File No.: 01669 File Date: 09/12/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 04/25/2014  
Solution Control Lot: 12D101 Bottle No.: 0567

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:04D		
Control 1 EC	0.100%	18:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:05D		
Control 2 EC	0.098%	18:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06D		
Control 3 EC	0.099%	18:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

## Changed By:

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 09/12/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01619	Calib. Date: 06/19/2013
Certification File No.:	01620	Calib. No.: 00027
Linearity File No.:	01621	Cert. Date: 06/19/2013
Solution File No.:	01659	Cert. No.: 00018
Sequential File No.:	01659	Lin. Date: 06/19/2013
		Lin. No.: 00017
		Soln. Date: 08/18/2013
		Soln. No.: 00183
		File Date: 08/18/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%	Expires:	04/25/2014	Bottle No.:	0562
Solution Control Lot:	12D101				

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:47D		
Control 1 EC	0.101%	19:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:48D		
Control 2 EC	0.100%	19:49D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	19:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:49D		
Control 3 EC	0.100%	19:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 08/18/2013

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01619 Calib. Date: 06/19/2013 Calib. No.: 00027  
Certification File No.: 01620 Cert. Date: 06/19/2013 Cert. No.: 00018  
Linearity File No.: 01621 Lin. Date: 06/19/2013 Lin. No.: 00017  
Solution File No.: 01644 Soln. Date: 07/29/2013 Soln. No.: 00182  
Sequential File No.: 01644 File Date: 07/29/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 04/25/2014  
Solution Control Lot: 12D101 Bottle No.: 0573

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:56D		
Control 1 EC	0.099%	03:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:57D		
Control 2 EC	0.098%	03:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:58D		
Control 3 EC	0.099%	03:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	03:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:59D		

All tests within acceptable tolerance.

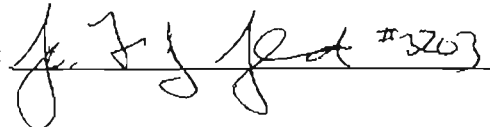
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature:  #3203

Badge No.: 3203

Date: 07/29/2013

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01619 Calib. Date: 06/19/2013 Calib. No.: 00027  
Certification File No.: 01620 Cert. Date: 06/19/2013 Cert. No.: 00018  
Linearity File No.: 01621 Lin. Date: 06/19/2013 Lin. No.: 00017  
Solution File No.: 01633 Soln. Date: 07/11/2013 Soln. No.: 00181  
Sequential File No.: 01633 File Date: 07/11/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 04/25/2014  
Solution Control Lot: 12D101 Bottle No.: 0574

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:05D		
Control 1 EC	0.100%	10:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:06D		
Control 2 EC	0.099%	10:07D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08D		
Control 3 EC	0.099%	10:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:09D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 07/11/2013



# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
Location: STRATFORD POLICE DEPT.  
Calibration File No.: 01487 Calib. Date: 01/10/2013 Calib. No.: 00026  
Certification File No.: 01488 Cert. Date: 01/10/2013 Cert. No.: 00017  
Linearity File No.: 01489 Lin. Date: 01/10/2013 Lin. No.: 00016  
Solution File No.: 01617 Soln. Date: 06/16/2013 Soln. No.: 00179  
Sequential File No.: 01617 File Date: 06/16/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
Control Solution %: 0.100% Expires: 04/25/2014  
Solution Control Lot: 12D101 Bottle No.: 0557

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:01D		
Control 1 EC	0.100%	19:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	19:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:02D		
Control 2 EC	0.099%	19:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	19:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:04D		
Control 3 EC	0.098%	19:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:05D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 06/16/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKJII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01487	Calib. Date: 01/10/2013
Certification File No.:	01488	Calib. No.: 00026
Linearity File No.:	01489	Cert. Date: 01/10/2013
Solution File No.:	01607	Cert. No.: 00017
Sequential File No.:	01607	Lin. Date: 01/10/2013
		Lin. No.: 00016
		Soln. Date: 06/01/2013
		Soln. No.: 00178
		File Date: 06/01/2013

Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %: 0.100%		Expires: 04/25/2014
Solution Control Lot: 12D101		Bottle No.: 0552

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	17:05D		
Control 1 EC	0.099%	17:06D	34.0°C	*** TEST PASSED ***
Control 1 1R	0.098%	17:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:07D		
Control 2 EC	0.097%	17:07D	34.0°C	*** TEST PASSED ***
Control 2 1R	0.097%	17:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:08D		
Control 3 EC	0.098%	17:08D	34.0°C	*** TEST PASSED ***
Control 3 1R	0.098%	17:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:09D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_



Badge No.: 3200

Date: 06/01/2013

# Calibrating Unit

## New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. No.:	00017
Linearity File No.:	01489	Lin. Date:	01/10/2013
Solution File No.:	01599	Soln. No.:	00177
Sequential File No.:	01599	File Date:	05/25/2013
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUK S3-0133
Solution Control Lot:	12DI01	Expires:	04/25/2014
		Bottle No.:	0553

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:14D		
Control 1 EC	0.098%	05:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	05:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:15D		
Control 2 EC	0.098%	05:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	05:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:17D		
Control 3 EC	0.097%	05:17D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	05:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:18D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KELLY

First Name: ROBERT

MI: J

Signature: 

# 

Badge No.: 3204

Date: 05/25/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. No.:	00026
Linearity File No.:	01489	Cert. Date:	01/10/2013
Solution File No.:	01587	Lin. No.:	00017
Sequential File No.:	01587	Lin. Date:	01/10/2013
		Soln. No.:	00176
		Soln. Date:	05/10/2013
		File Date:	05/10/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	04/25/2014
Solution Control Lot:	12D101			Bottle No.:	0551

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:41D		
Control 1 EC	0.098%	11:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	11:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:42D		
Control 2 EC	0.098%	11:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:43D		
Control 3 EC	0.098%	11:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KELLY

First Name: ROBERT

M1: J

Signature: \_\_\_\_\_

*Sgt. R Kelly*

# 3204

Badge No.: 3204

Date: 05/10/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. Date:	01/10/2013
Linearity File No.:	01489	Lin. Date:	01/10/2013
Solution File No.:	01573	Soln. Date:	04/22/2013
Sequential File No.:	01573	File Date:	04/22/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	04/25/2014
Solution Control Lot:	12D101			Bottle No.:	0558

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	14:31D		
Control 1 EC	0.100%	14:32D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:32D		
Control 2 EC	0.098%	14:33D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	14:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:34D		
Control 3 EC	0.098%	14:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	14:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:35D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  63201

Badge No.: 3200

Date: 04/22/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. Date:	01/10/2013
Linearity File No.:	01489	Lin. Date:	01/10/2013
Solution File No.:	01572	Soln. Date:	04/22/2013
Sequential File No.:	01572	File Date:	04/22/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	04/25/2014
Solution Control Lot:	12D101			Bottle No.:	0561

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:24D		
Control 1 EC	-.---%	12:25D	22.2°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	12:25D	22.2°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	---:---		
Control 2 EC	-.---%	---:---	N/A	
Control 2 IR	-.---%	---:---	N/A	
Ambient Air Blank	-.---%	---:---		
Control 3 EC	-.---%	---:---	N/A	
Control 3 IR	-.---%	---:---	N/A	
Ambient Air Blank	-.---%	---:---		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

Badge No.: 3200

Date: 04/22/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. Date:	01/10/2013
Linearity File No.:	01489	Lin. Date:	01/10/2013
Solution File No.:	01567	Soln. Date:	04/15/2013
Sequential File No.:	01567	File Date:	04/15/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	04/25/2014
Solution Control Lot:	12D101			Bottle No.:	0559

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:55D		
Control 1 EC	0.099%	01:56D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	01:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:56D		
Control 2 EC	0.097%	01:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	01:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:58D		
Control 3 EC	0.098%	01:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	01:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:59D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: GAGLIARDI

First Name: FRANK

MI: J

Signature:  #3203

Badge No.: 3203

Date: 04/15/2013

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01487	Calib. Date: 01/10/2013
Certification File No.:	01488	Calib. No.: 00026
Linearity File No.:	01489	Cert. Date: 01/10/2013
Solution File No.:	01558	Cert. No.: 00017
Sequential File No.:	01558	Lin. Date: 01/10/2013
		Lin. No.: 00016
		Soln. Date: 04/10/2013
		Soln. No.: 00172
		File Date: 04/10/2013

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDUK S3-0133
Control Solution %:	0.100%		Expires: 04/25/2014
Solution Control Lot:	12D101		Bottle No.: 0554

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:30D		
Control 1 EC	0.099%	10:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:32D		
Control 2 EC	0.098%	10:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:33D		
Control 3 EC	0.098%	10:34D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE CROSS SERIAL NUMBER: DDUK S3-0015 (MPA)

Changed By:

Last Name: GIBSON

First Name: MICHAEL

MI: P

Signature:

*Michael P. Gibson #6353*

Badge No.: 6353

Date: 04/10/2013





**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Serial Number:

Model: MARK IIA

DDUK 53-0133

Other: \_\_\_\_\_

Certification Date

Technician

Re-Certification Due Date

1-17-2013

BC

1-17-2014

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date

Next Certification due:

DDLLPI-0015

1-17-2013

1-17-2014

Probe Value

105

Dräger Safety Diagnostics, Inc.  
Technical Service Department

BC

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01487	Calib. Date:	01/10/2013
Certification File No.:	01488	Cert. No.:	00026
Linearity File No.:	01489	Cert. No.:	00017
Solution File No.:	01546	Lin. Date:	01/10/2013
Sequential File No.:	01546	Lin. No.:	00016
		Soln. Date:	03/28/2013
		Soln. No.:	00171
		File Date:	03/28/2013
<b>Calibrating Unit:</b>	WET	Model No.	CU-34
Control Solution %:	0.100%	Serial No.:	DDUL S2-0163
Solution Control Lot:	12D101	Expires:	04/25/2014
		Bottle No.:	0563

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:53S		
Control 1 EC	0.098%	10:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	10:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55S		
Control 2 FC	0.097%	10:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:56S		
Control 3 EC	0.098%	10:57S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:58S		

All tests within acceptable tolerance

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI M

Signature: 

Badge No.: 3200

Date: 03/28/2013

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
 Location: STRATFORD POLICE DEPT.  
 Calibration File No.: 01487 Calib. Date: 01/10/2013 Calib. No.: 00026  
 Certification File No.: 01488 Cert. Date: 01/10/2013 Cert. No.: 00017  
 Linearity File No.: 01489 Lin. Date: 01/10/2013 Lin. No.: 00016  
 Solution File No.: 01526 Soln. Date: 03/08/2013 Soln. No.: 00170  
 Sequential File No.: 01526 File Date: 03/08/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUL S3-0163  
 Control Solution %: 0.100% Expires: 04/25/2014  
 Solution Control Lot: 12D101 Bottle No.: 0570

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:21S		
Control 1 EC	0.100%	10:22S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:22S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:23S		
Control 2 EC	0.099%	10:24S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:24S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:24S		
Control 3 EC	0.099%	10:25S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:25S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:26S		

All tests within acceptable tolerance.

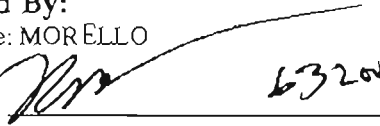
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature:  6320

Badge No.: 3200

Date: 03/08/2013

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location	STRATFORD POLICE DEPT.	
Calibration File No.:	01487	Calib. No.: 00026
Certification File No.:	01488	Cert. No.: 00017
Linearity File No.:	01489	Lin. No.: 00016
Solution File No.:	01514	Soln. No.: 00169
Sequential File No.:	01514	File Date: 02/16/2013
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUT 53-0163
Solution Control Lot:	12D101	Expires: 04/25/2014
		Bottle No.: 0560

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:41S		
Control 1 EC	0.097%	18:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:42S		
Control 2 EC	0.097%	18:43S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:43S		
Control 3 EC	0.098%	18:44S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:44S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:45S		

All tests within acceptable tolerance

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: KELLY

First Name: ROBERT

MJJ

Signature: 

# 304

Badge No.: 3204

Date: 02/16/2013

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0039
Location:	STRATFORD POLICE DEPT.	
Calibration File No.:	01487	Calib. Date: 01/10/2013
Certification File No.:	01488	Calib. No.: 00026
Linearity File No.:	01489	Cert. Date: 01/10/2013
Solution File No.:	01502	Cert. No.: 00017
Sequential File No.:	01502	Lin. Date: 01/10/2013
		Lin. No.: 00016
		Soln. Date: 01/28/2013
		Soln. No.: 00168
		File Date: 01/28/2013

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUL S3-0163
Solution Control Lot:	12D101	Expires: 04/25/2014
		Bottle No.: 0555

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:06S		
Control 1 EC	0.099%	10:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:07S		
Control 2 EC	0.098%	10:08S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:08S		
Control 3 EC	0.099%	10:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:10S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: \_\_\_\_\_

 63200

Badge No.: 3200

Date: 01/28/2013

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0039  
 Location: STRATFORD POLICE DEPT.  
 Calibration File No.: 01340 Calib. Date: 08/07/2012 Calib. No.: 00025  
 Certification File No.: 01341 Cert. Date: 08/07/2012 Cert. No.: 00016  
 Linearity File No.: 01342 Lin. Date: 08/07/2012 Lin. No.: 00015  
 Solution File No.: 01486 Soln. Date: 01/09/2013 Soln. No.: 00166  
 Sequential File No.: 01486 File Date: 01/09/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUK S3-0133  
 Control Solution %: 0.100% Expires: 04/25/2014  
 Solution Control Lot: 12D101 Bottle No.: 0565

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:31S		
Control 1 EC	-.---%	12:31S	38.7°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	12:31S	38.7°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 01/09/2013

# Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKII-C	Serial No.:	ARNK-0039
Location:	STRATFORD POLICE DEPT.		
Calibration File No.:	01340	Calib. Date:	08/07/2012
Certification File No.:	01341	Cert. No.:	00025
Linearity File No.:	01342	Cert. Date:	08/07/2012
Solution File No.:	01485	Lin. No.:	00015
Sequential File No.:	01485	Lin. Date:	08/07/2012
		Soln. No.:	00165
		Soln. Date:	01/09/2013
		File Date:	01/09/2013

Calibrating Unit:	WET	Model No.:	CU-14	Serial No.:	DDUK S3-0133
Control Solution %:	0.100%			Expires:	04/25/2014
Solution Control Lot:	12D101			Bottle No.:	0568

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:45S		
Control 1 EC	.....%	10:45S	37.9°C	SIMULATOR TEMP. ERROR
Control 1 IR	.....%	10:45S	37.9°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	.....%	-----		
Control 2 EC	.....%	-----	N/A	
Control 2 IR	.....%	-----	N/A	
Ambient Air Blank	.....%	-----		
Control 3 EC	.....%	-----	N/A	
Control 3 IR	.....%	-----	N/A	
Ambient Air Blank	.....%	-----		

Test results are not within acceptable range.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: MORELLO

First Name: RONALD

MI: M

Signature: 

Badge No.: 3200

Date: 01/09/2013