

# ALCOTEST CHECKLIST

Municipality: WESTAMPTON TWP. Alcotest Ser. #: ARNK-0025

County: BURLINGTON Date of Calibration: 11-15-2012

- 1. **Certificate of Accuracy Alcotest 7110 MKIII-C** from Draeger Safety for instrument used in the A.I.R.
- 2. **Certificate of Accuracy CU34 Unit** on Alcotest Instrument used.  
Ser. #: DDUJ 53-0117
- 3. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety for instrument in A.I.R. or equivalent.  
Ser. #: DDWA P2-116
- 4. **Digital Temperature Measuring System Report of Calibration.**  
Ser. #: 122172 176
- 5.
  - A. Alcotest 7110 Calibration Record
  - B. Alcotest 7110 Calibration Certificate **Part I - Control Tests.**
  - C. Alcotest 7110 Calibration Certificate **Part II - Linearity Tests.**
  - D. **Alcotest Card** of operator/coordinator who performed tests.
  - E. **Certificate of Accuracy Alcotest 7110 Temperature Probe** from Draeger Safety used in the Calibration Tests ["Black Key" probe of Breath Test Coordinator].  
Ser. #: DDMB P1-0002
- 6. **Certificates of Analysis** for each **Simulator Solution** used in Calibration/Linearity Tests:
  - A. 0.04% Solution. 11 F 090
  - B. 0.08% Solution. 11 F 091
  - C. 0.10% Solution. 12 B 099
  - D. 0.16% Solution. 11 G 092
- 7. Certificate of Accuracy Alcotest CU34 Simulators from Draeger Safety (when conducting the Calibration/Linearity Tests) for:
  - A. 0.04% used in Calibration/Linearity Testing. DDWF 53-0215
  - B. 0.08% used in Calibration/Linearity Testing. DDXD 53-0193
  - C. 0.10% used in Calibration/Linearity Testing DDUJ 53-0117  
[Same as instrument's CU34 unit].
  - D. 0.16% used in Calibration/Linearity Testing. DDWF 53-0241
- 8.
  - A. New Standard Solution Report following Calibration.
  - B. Calibrating CU34 Unit for same [same as CU34 unit on instrument].
  - C. Certificate of Analysis 0.10% solution for same.  
Lot #: 11 A 085
  - D. Alcotest card of operator/coordinator who completed change.

**Dräger**safety

**Alcotest<sup>®</sup> 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

7-8-09

ARNK-0025

**Draeger Safety Diagnostics, Inc.**

\_\_\_\_\_ *JS*



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDUJS3-0117

Certification Date

Technician

Re-Certification Due Date

3/16/12

ZM

3/16/13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWA P2-116

3/16/12

3/16/13

Probe Value

103

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

ZM



Calibration  
Certificate No. 1750.01

Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-4269985

**Traceable® Certificate of Calibration for Digital Thermometer**

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087  
**Instrument Identification:**

Model: 61220-601      S/N: 122172178      Manufacturer: Control Company

**Standards/Equipment:**

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	ASA237		
Digital Thermometer	B16815	8/06/12	B1606038
PRT Temperature Probe	01841	5/28/12	B1526085
Temperature Calibration Bath TC-256	B01375		
Thermistor Module	A27129	10/31/12	1000306945
Temperature Probe	157	11/13/12	6-BL72N-1-1
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	2/01/13	1000311439
Temperature Probe	128	2/14/13	6-BN9WZ-27-1

**Certificate Information:**

Technician: 68      Procedure: CAL-08      Cal Date: 3/30/12      Cal Due: 3/30/14  
Test Conditions: 23.0°C      44.0 %RH      1012 mBar

**Calibration Data: (New Instrument)**

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.001	Y	-0.050	0.050	0.019	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.014	3.6:1
°C		N.A.		99.999	99.999	Y	99.950	100.050	0.018	2.8:1
°C		N.A.		100.001	100.002	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; MH = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YYYY

*Ricard Rodriguez*  
Ricard Rodriguez, Quality Manager

*Wallace Berry*  
Wallace Berry, Technical Manager

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-8448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation (ILAC) - MRA Mutual Recognition Arrangement (MRA).

# Alcotest 7110 Calibration Record

**Equipment**

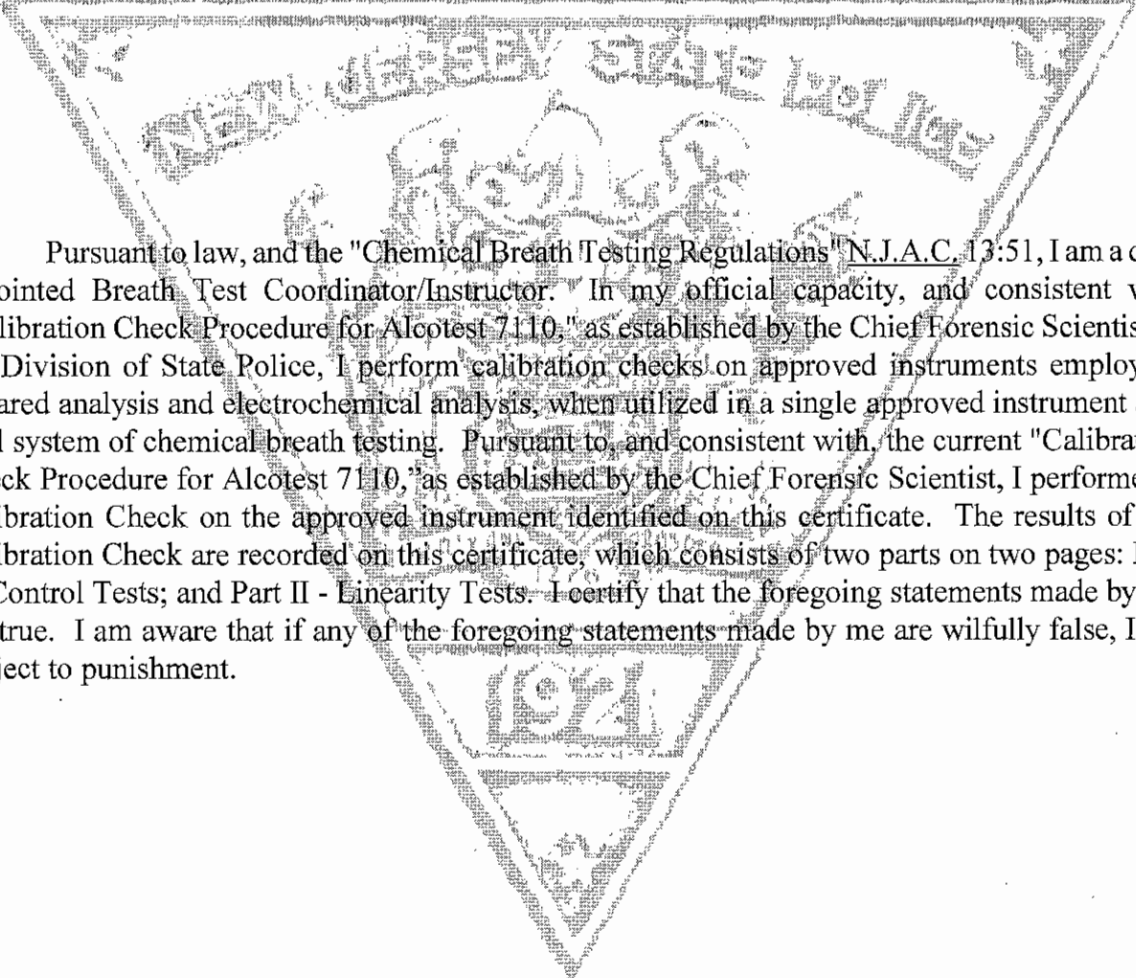
Alcotest 7110 MKIII-C  
Serial No.: ARNK-0025  
Location: WESTAMPTON POLICE  
Calibration File No.: 00492  
Calib. Date: 11/15/2012  
Calib. No.: 00016  
Certification File No.: 00472  
Cert. Date: 06/05/2012  
Cert. No.: 00012  
Linearity File No.: 00473  
Lin. Date: 06/05/2012  
Lin. No.: 00013  
Solution File No.: 00491  
Soln. Date: 11/07/2012  
Soln. No.: 00121  
Sequential File No.: 00492  
File Date: 11/15/2012

Calibrating Unit: WET  
Model No.: CU-34  
Serial No.: DDUJ S3-0117  
Control Solution %: 0.100%  
Expires: 02/20/2014  
Solution Control Lot: 12B099  
Bottle No.: 0021

**Coordinator**

Last Name: GONCALVES  
First Name: MICHELLE  
MI: L  
Signature: Det I. Alves #6040  
Badge No.: 6040  
Date: 11/15/2012

\*Black Key Temperature Probe Serial.....# DDMBP1-0002 (MIA)  
\*Digital NIST Temperature Measuring System Serial.....# 122172176 (MIA)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0025  
Location: WESTAMPTON POLICE  
Calibration File No.: 00492 Calib. Date: 11/15/2012 Calib. No.: 00016  
Certification File No.: 00493 Cert. Date: 11/15/2012 Cert. No.: 00013  
Linearity File No.: 00473 Lin. Date: 06/05/2012 Lin. No.: 00013  
Solution File No.: 00491 Soln. Date: 11/07/2012 Soln. No.: 00121  
Sequential File No.: 00493 File Date: 11/15/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUJ S3-0117  
Control Solution %: 0.100% Expires: 02/20/2014  
Solution Control Lot: 12B099 Bottle No.: 0021

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:54S		
Control 1 EC	0.099%	09:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56S		
Control 2 EC	0.097%	09:56S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:57S		
Control 3 EC	0.098%	09:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59S		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: *Michelle Goncalves*

Badge No.: 6040

Date: 11/15/2012

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARNK-0025  
Location: WESTAMPTON POLICE  
Calibration File No.: 00492 Calib. Date: 11/15/2012 Calib. No.: 00016  
Certification File No.: 00493 Cert. Date: 11/15/2012 Cert. No.: 00013  
Linearity File No.: 00494 Lin. Date: 11/15/2012 Lin. No.: 00014  
Solution File No.: 00491 Soln. Date: 11/07/2012 Soln. No.: 00121  
Sequential File No.: 00494 File Date: 11/15/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0215  
Control Solution %: 0.040% Expires: 06/27/2013  
Solution Control Lot: 11F090 Bottle No.: 1226

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0193  
Control Solution %: 0.080% Expires: 06/30/2013  
Solution Control Lot: 11F091 Bottle No.: 0941

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0241  
Control Solution %: 0.160% Expires: 07/03/2013  
Solution Control Lot: 11G092 Bottle No.: 0426

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:09S		
Control 1 EC	0.042%	10:10S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	10:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:11S		
Control 2 EC	0.040%	10:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	10:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13S		
Control 3 EC	0.080%	10:14S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	10:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16S		
Control 4 EC	0.079%	10:16S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.078%	10:16S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:18S		
Control 5 EC	0.159%	10:18S	34.0°C	*** TEST PASSED ***
Control 5 IR	0.160%	10:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20S		
Control 6 EC	0.158%	10:21S	34.0°C	*** TEST PASSED ***
Control 6 IR	0.159%	10:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22S		

All tests within acceptable tolerance.

### Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: \_\_\_\_\_

*Det I. Alves #6040*

Badge No.: 6040

Date: 11/15/2012



# CERTIFICATE

This is to certify that

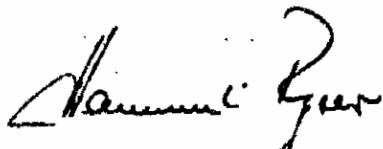
**Michelle Goncalves**

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and  
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012

  
\_\_\_\_\_  
Instructor: Hansueli Ryser

**Dräger**





CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lieutenant Governor

*State of New Jersey*  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF CRIMINAL JUSTICE  
PO BOX 085  
TRENTON, NJ 08623-0085  
TELEPHONE: (609) 984-6500

JEFFREY S. CHIESA  
Attorney General

STEPHEN J. TAYLOR  
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent  
Division of State Police  
Division Headquarters  
P.O. Box 7068  
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -  
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C. 13:51-2.1 (b) and (c)*, as adopted and promulgated under the provisions of *N.J.S.A. 39:4-50.3, 39:3-10.25 and 12:7-56*, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa  
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police  
DSFC Patrick Guilfooy, Unit Head, Alcohol/Drug Test Unit, Division of State Police ✓



DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michael L. McKelvey**  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 BY THE OPERATION OF THE **Breathalyzer**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **16th** DAY OF **Aug.**  
TWO THOUSAND AND **04**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES Feb. 3-7-2003

Refresher Course

DATE	PLACE	INSTRUCTOR
1. <u>10/10/03</u>	<u>OCPA</u>	<u>[Signature]</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**MICHELLE L. MCKELVEY**  
NEW JERSEY STATE POLICE  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 BY THE OPERATION OF THE **ALCOHOL 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **10th** DAY OF **August**  
TWO THOUSAND AND **FIVE**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michelle L. Goncalves**  
New Jersey State Police  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 BY THE OPERATION OF THE **ALCOHOL 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **15th** DAY OF **December**  
TWO THOUSAND AND **EIGHT**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that  
**Michelle Goncalves**  
New Jersey State Police  
IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 BY THE OPERATION OF THE **Breath Test Coordinator/Instructor**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **23rd** DAY OF **March**  
TWO THOUSAND AND **Twelve**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 283B (Rev. 05/02)



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 West Trenton NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

PAULA T. DOW  
 Attorney General

KIM GUADAGNO  
 Lt. Governor

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

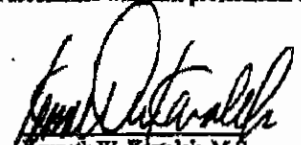
MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F090

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Kowalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

  
 Notary

Linda S. Bellantieri  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 West Trenton NJ 08625-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

PAULA T. DOW  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc. ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11E091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13-51-3.4, of approved breath test instruments (N.J.A.C. 13-51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Krwalick, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

Notary

Linda L. Desantis  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON, NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
*Governor*

JEFFREY S. CHIESA  
*Attorney General*

KIM GUADAGNO  
*Lt. Governor*

COLONEL JOSEPH R. FUENTES  
*Superintendent*

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 3/20/2012

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 12B099

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1207 to 0.1211 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 20, 2014.

As Forensic Scientist III for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Monica L. Tramontin  
 Forensic Scientist III  
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20<sup>th</sup> day of March, 2012.

Notary

MARY ELIZABETH MCLAUGHLIN  
 NOTARY PUBLIC OF NEW JERSEY  
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 Post Office Box 7068  
 West Trenton NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

PAULA T. DOW  
 Attorney General

KIM GUADAGNO  
 Lt. Governor

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

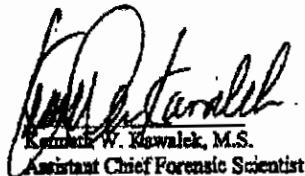
MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 7/25/2011


BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Kawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.  
  
 Notary

  
 Linda L. Wiantis  
 Notary Public, New Jersey  
 My Commission Expires 0-17-11



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWFS3-0241

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDWFS3-0215

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13



**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

012X053-0193

Certification Date

Technician

Re-Certification Due Date

8-6-12

AS

8-6-13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDMBP1-0002

2/3/12

2/3/13

Probe Value

10.2

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

2M



# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0025
Location:	WESTAMPTON POLICE		
Calibration File No.:	00492	Calib. Date:	11/15/2012
Certification File No.:	00493	Cert. No.:	00016
Linearity File No.:	00494	Cert. Date:	11/15/2012
Solution File No.:	00495	Lin. No.:	00014
Sequential File No.:	00495	Soln. Date:	11/15/2012
		Soln. No.:	00122
		File Date:	11/15/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUJ S3-0117
Solution Control Lot:	11A085	Expires:	01/20/2013
		Bottle No.:	0809

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:31S		
Control 1 EC	0.101%	11:32S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33S		
Control 2 EC	0.099%	11:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:34S		
Control 3 EC	0.099%	11:35S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number DDWAP2-116 KIC

**Changed By:**

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: Det I Galves #6040

Badge No.: 6040

Date: 11/15/2012



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

PAULA T. DOW  
 Attorney General

KIM GUADAGNO  
 Lt. Governor

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

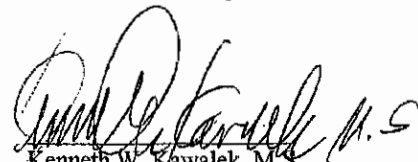
**ANALYSIS DATE:** 2/11/2011

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 11A085


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1201 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 20, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
 Kenneth W. Kawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 15<sup>th</sup> day of February, 2011.

  
 Notary

**Linda L. Desantis**  
 Notary Public, New Jersey  
 My Commission Expires 6-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable

